

Medtronic




Only Evolut™ TAVI outperforms SAVR in younger, low risk patients.^{†1}

Clinical implications from late-breaking evidence presented at TCT 2023:

In younger, low risk patients, the Evolut platform is the THV of first choice due to excellent clinical outcomes.¹

Primary Endpoint: All-Cause Mortality or Disabling Stroke

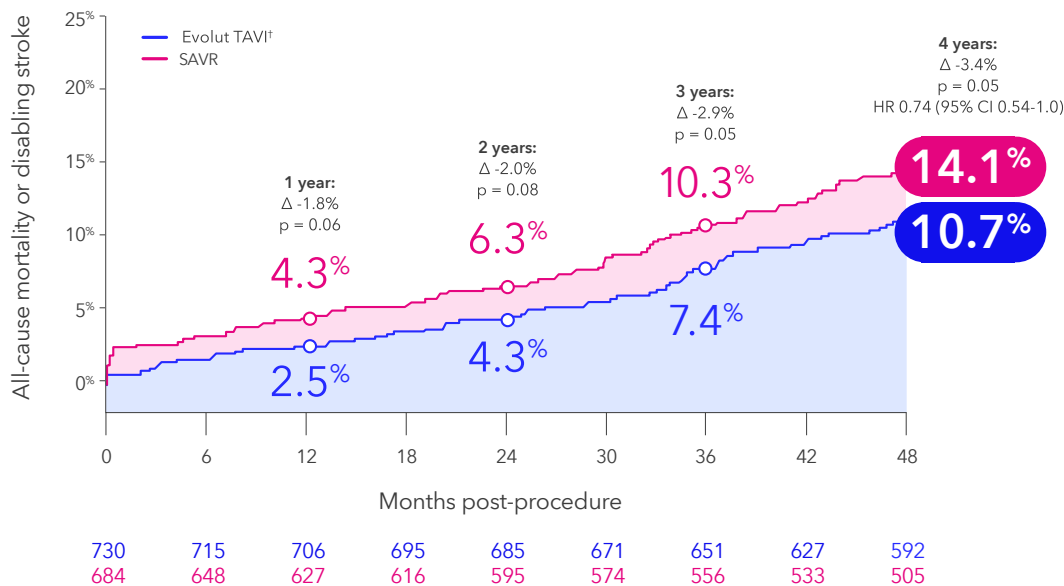

Difference in Kaplan-Meier rates broadened over time

Reduction in hazard for death or disabling stroke at 4 years.¹

26%

[†]Devices: Evolut R 73%/Evolut PRO 23.4%/CoreValve™ 3.6%.

¹Reardon M, et al. Transcatheter Versus Surgical Aortic Valve Replacement in Aortic Stenosis Patients at Low Surgical Risk: 4-Year Outcomes from the Evolut Low Risk Trial. Presented at TCT; October 2023.

See the CoreValve™ Evolut™ R, the CoreValve™ Evolut™ PRO, the Evolut™ PRO+ device and the Evolut™ FX device manuals for detailed information regarding the instructions for use, the implant procedure, indications, contraindications, warnings, precautions, and potential adverse events. For further information, contact your local Medtronic representative and/or consult the Medtronic website at medtronic.eu. For applicable products, consult instructions for use on manuals.medtronic.com. Manuals can be viewed using a current version of any major internet browser. For best results, use Adobe Acrobat™ Reader with the browser. The commercial name of the Evolut™ R device is Medtronic CoreValve™ Evolut™ R System, the commercial name of the Evolut™ PRO device is Medtronic CoreValve™ Evolut™ PRO System, the commercial name of the Evolut™ PRO+ device is Medtronic Evolut™ PRO+ System, and the commercial name of the Evolut™ FX device is Medtronic Evolut™ FX System.

CE
0344

Medtronic

Europe

Medtronic International Trading Sàrl.
Route du Molliau 31
Case postale
CH-1131 Tolochenaz
medtronic.com

©2023 Medtronic. All rights reserved. Medtronic, Medtronic logo, and Engineering the extraordinary are trademarks of Medtronic. All other brands are trademarks of a Medtronic company.

UC202311218a EE
10/2023